


Thermo Nicolet

Title: L# 169568B Chondroitin Sulfate

Number of sample scans: 32
Number of background scans: 32
Resolution: 8.000
Sample gain: 16.0
Mirror velocity: 0.6329
Aperture: 1.00

Detector: Unknown
Beamsplitter: KBr
Source: IR

Comment:

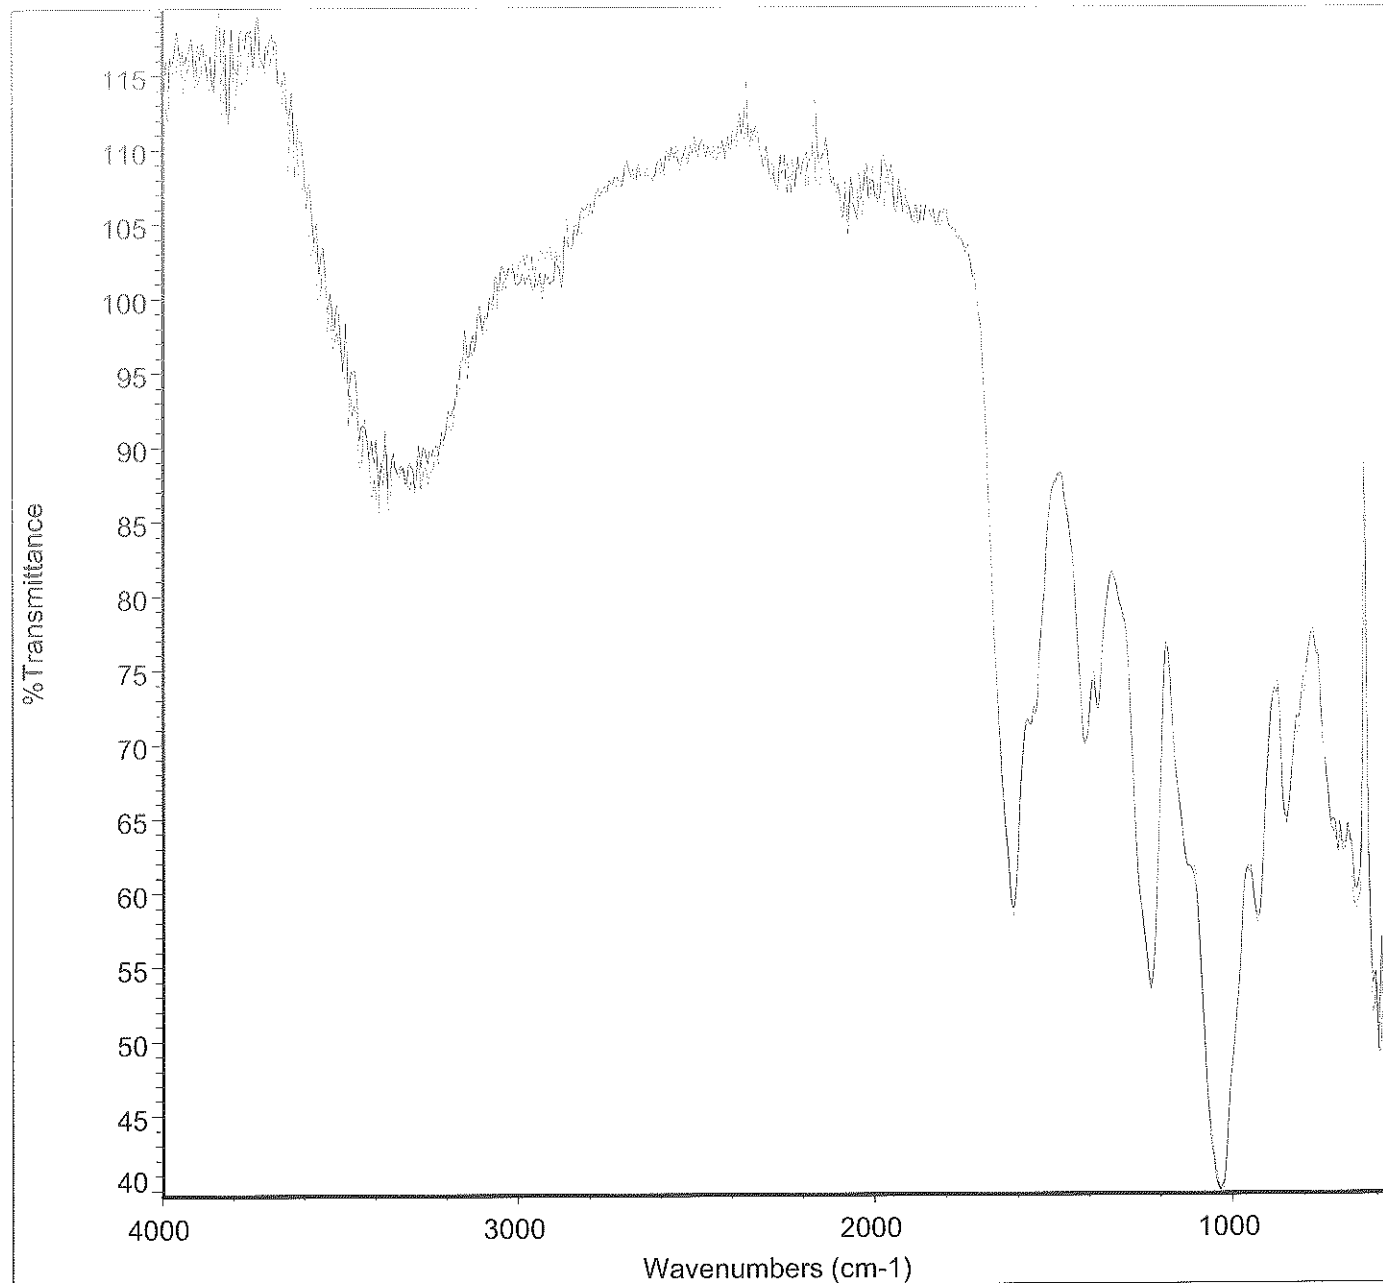

Thermo Nicolet

Title: Chondroitin Sulfate Std 8

Number of sample scans: 32
Number of background scans: 32
Resolution: 8.000
Sample gain: 16.0
Mirror velocity: 0.6329
Aperture: 1.00

Detector: Unknown
Beamsplitter: KBr
Source: IR

Comment:

