

Single Mass Analysis

Tolerance = 5.0 PPM / DBE: min = -1.5, max = 50.0

Element prediction: Off

Number of isotope peaks used for i-FIT = 4

Monoisotopic Mass, Even Electron Ions

2382 formula(e) evaluated with 4 results within limits (all results (up to 1000) for each mass)


Elements Used:

C: 0-500 H: 0-200 N: 0-200 O: 0-200 Na: 0-1 Si: 0-1 S: 0-6 Ca: 0-5

KBL_500_001

KBL_500_001 32 (0.528) Cm (27:38)

TOF MS ES+
2.46e+004

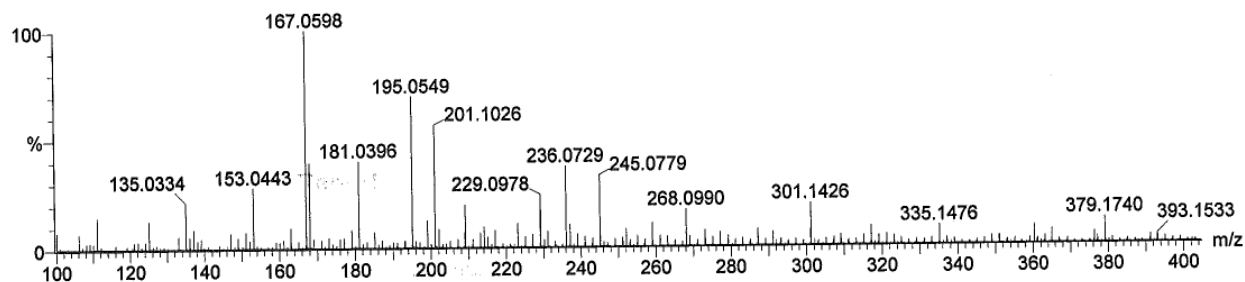

Minimum: -1.5
Maximum: 5.0 5.0 50.0

Mass	Calc. Mass	mDa	PPM	DBE	i-FIT	i-FIT (Norm)	Formula
195.0549	195.0550	-0.1	-0.5	1.5	636.2	4.5	C3 H11 N4 O4 Si
	195.0552	-0.3	-1.5	1.5	633.7	2.1	C4 H11 N4 O3 S
	195.0545	0.4	2.1	-1.5	631.8	0.2	C5 H15 O5 Ca
	195.0558	-0.9	-4.6	10.5	636.9	5.2	C12 H7 N2 O

Single Mass Analysis

Tolerance = 5.0 PPM / DBE: min = -1.5, max = 50.0

Element prediction: Off

Number of isotope peaks used for i-FIT = 4

Monoisotopic Mass, Even Electron Ions

1311 formula(e) evaluated with 2 results within limits (all results (up to 1000) for each mass)


Elements Used:

C: 0-500 H: 0-200 N: 0-200 O: 0-200 Na: 0-1 Si: 0-1 S: 0-6 Ca: 0-5

KBL_500_001

KBL_500_001 32 (0.528) Cm (27:38)

TOF MS ES+
2.46e+004

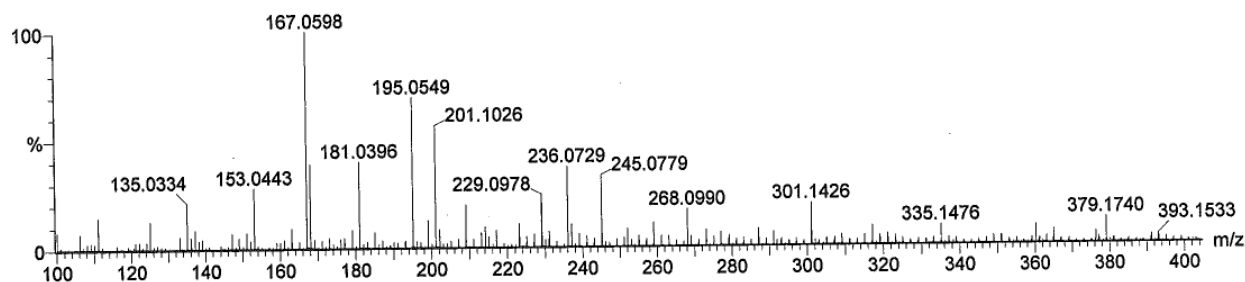

Minimum: -1.5
Maximum: 5.0 5.0 50.0

Mass	Calc. Mass	mDa	PPM	DBE	i-FIT	i-FIT (Norm)	Formula
167.0598	167.0600	-0.2	-1.2	0.5	721.0	5.6	C2 H11 N4 O3 Si
	167.0603	-0.5	-3.0	0.5	715.3	0.0	C3 H11 N4 O2 S